


SEATING TISSUE LOAD MANAGEMENT ALGORITHM

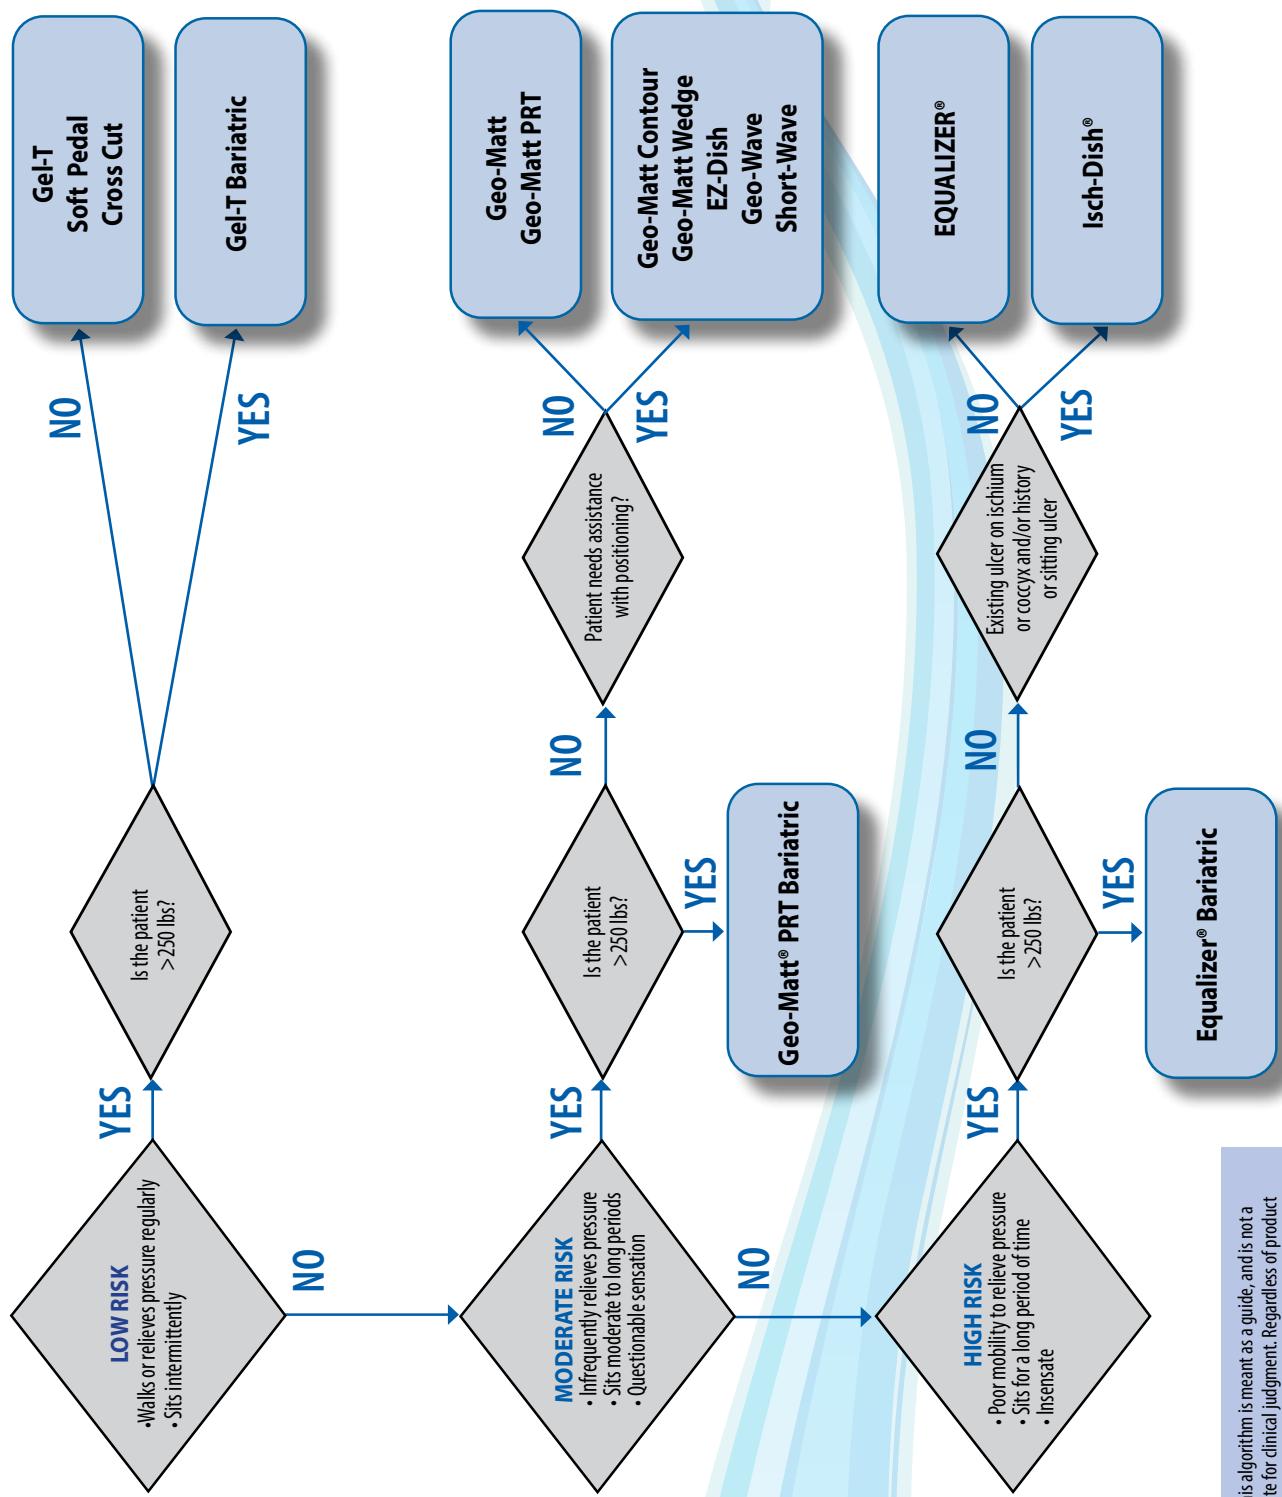

Note: This algorithm is meant as a guide, and is not a substitute for clinical judgment. Regardless of product selection, a full assessment of skin status and repositioning is required according to best clinical practice.